


<< Titration result >>

Sample No.	: 07-11	Date	: 2017/09/12 17:08:15
Model	: MKC-710(MCU-710)	Time	: 00:01:20
Serial No.	: 20270615		
Operator	:		
Method name	: Sample		
Anolyte Reagent Name	: Anolyte	Anolyte Life Value	: 15 mg
Catholyte Reagent Name	: Catholyte	Catholyte Life Value	: 15 mg
Drift Stop Rel.	: 0.10 ug/s	Control gain	: 5.0
t(stir)	: 0 s	t(wait)	: 15 s
t(max)	: 0 s	Cell type	: 2-Comp.
Option	: Off	Oven temp.	: --- Deg.C
Pre-Treat	: -	Back purge	: ---- s
Cell purge	: ---- s	Sample purge	: ---- s
Calc.No.	: 2		
Sample name	: Methanol		
Sample ID	: 20170912	Size(Size) *	: 0.7526 g
Size(Wt1) *	: 0.7526 g	Size(Wt2) *	: 0.0000 g
Blank (Blank)	: 0.0000 ug	Revision Coef. (FA)	: 1.00000
Dissolve Samp. (Wt0)	: ---- g	Conc.of Solvent (A)	: ---- ppm
Dissolve Solvent (B)	: ---- g		
Samp.Volume (V1)	: ---- mL	Samp.Dens. (Dens)	: ---- g/mL
Samp.Gas Volume (V2)	: ---- L	Samp.Gas Temp. (Temp.)	: -- Deg.C
Recalculation comment	:		
[Result]			
Conc.	: 0.0251 %		
Moisture	: 189.0 ug	Drift	: 0.06 ug/s
Detection temp.	: --- Deg.C		

[Titration Curve]

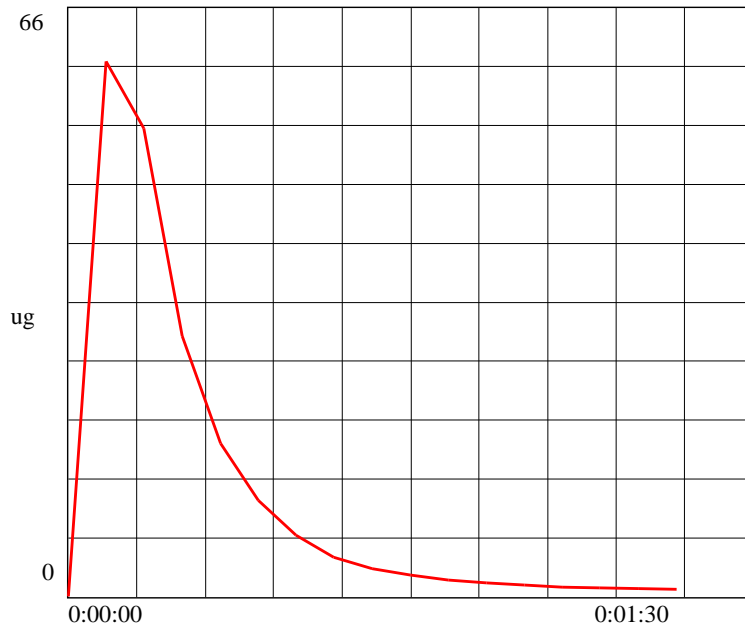


<< Titration result >>

Sample No. : 07-12 Date : 2017/09/12 17:13:34
 Model : MKC-710(MCU-710) Time : 00:01:20
 Serial No. : 20270615
 Operator :

Method name : Sample
 Anolyte Reagent Name : Anolyte Anolyte Life Value : 15 mg
 Catholyte Reagent Name : Catholyte Catholyte Life Value : 15 mg
 Drift Stop Rel. : 0.10 ug/s Control gain : 5.0
 t(stir) : 0 s t(wait) : 15 s
 t(max) : 0 s Cell type : 2-Comp.
 Option : Off Oven temp. : --- Deg.C
 Pre-Treat : - Back purge : ---- s
 Cell purge : ---- s Sample purge : ---- s
 Calc.No. : 2
 Sample name : Methanol
 Sample ID : 20170912 Size(Size) * : 0.7440 g
 Size(Wt1) * : 0.7440 g Size(Wt2) * : 0.0000 g
 Blank (Blank) : 0.0000 ug Revision Coef. (FA) : 1.00000
 Dissolve Samp. (Wt0) : ---- g Conc.of Solvent (A) : ---- ppm
 Dissolve Solvent (B) : ---- g
 Samp.Volume (V1) : ---- mL Samp.Dens. (Dens) : ---- g/mL
 Samp.Gas Volume (V2) : ---- L Samp.Gas Temp. (Temp.) : --- Deg.C
 Recalculation comment :

[Result]
 Conc. : 0.0253 %
 Moisture : 188.3 ug Drift : 0.06 ug/s
 Detection temp. : --- Deg.C


[Titration Curve]

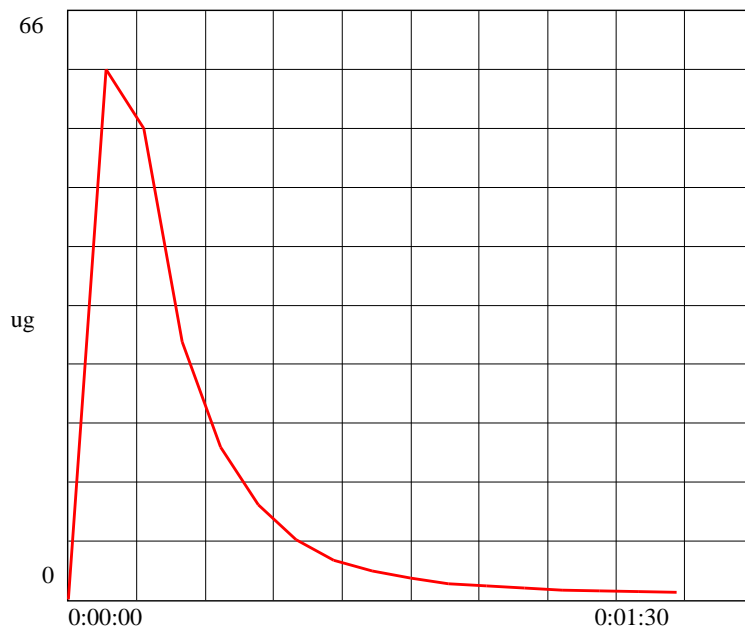

<< Titration result >>

Sample No.	: 07-13	Date	: 2017/09/12 17:15:59
Model	: MKC-710(MCU-710)	Time	: 00:01:11
Serial No.	: 20270615		
Operator	:		
Method name	: Sample		
Anolyte Reagent Name	: Anolyte	Anolyte Life Value	: 15 mg
Catholyte Reagent Name	: Catholyte	Catholyte Life Value	: 15 mg
Drift Stop Rel.	: 0.10 ug/s	Control gain	: 5.0
t(stir)	: 0 s	t(wait)	: 15 s
t(max)	: 0 s	Cell type	: 2-Comp.
Option	: Off	Oven temp.	: --- Deg.C
Pre-Treat	: -	Back purge	: ---- s
Cell purge	: ---- s	Sample purge	: ---- s
Calc.No.	: 2		
Sample name	: Methanol		
Sample ID	: 20170912	Size(Size) *	: 0.7445 g
Size(Wt1) *	: 0.7445 g	Size(Wt2) *	: 0.0000 g
Blank (Blank)	: 0.0000 ug	Revision Coef. (FA)	: 1.00000
Dissolve Samp. (Wt0)	: ---- g	Conc.of Solvent (A)	: ---- ppm
Dissolve Solvent (B)	: ---- g		
Samp.Volume (V1)	: ---- mL	Samp.Dens. (Dens)	: ---- g/mL
Samp.Gas Volume (V2)	: ---- L	Samp.Gas Temp. (Temp.)	: -- Deg.C
Recalculation comment	:		
[Result]			
Conc.	: 0.0251 %		
Moisture	: 186.9 ug	Drift	: 0.09 ug/s
Detection temp.	: --- Deg.C		

[Titration Curve]

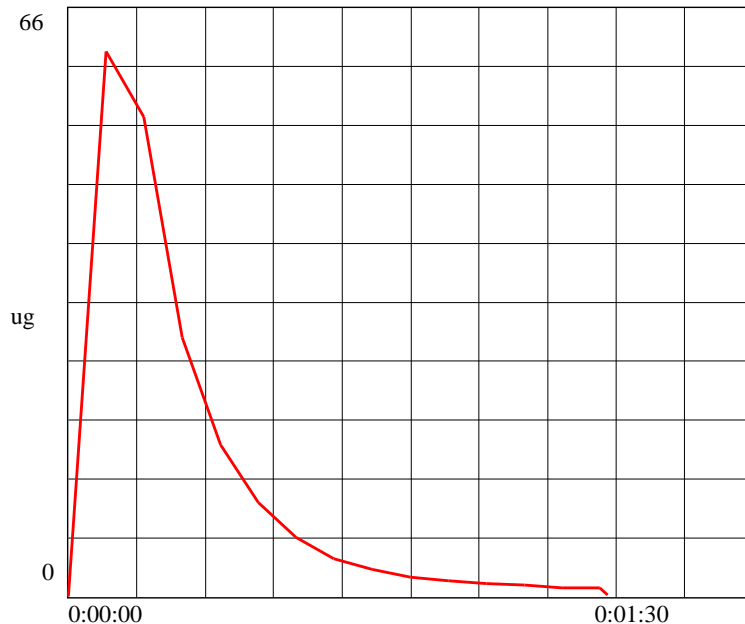

-Measurement results-

Run	Sample size (g)	Moisture(μg)	Conc. (%)	Statistics	
1	0.7526	189.0	0.0251	Mean	0.0252%
2	0.7440	188.3	0.0253	SD	0.0001%
3	0.7445	186.9	0.0251	RSD	0.3968%